



October 21, 2026

Kansas Department of Health and Environment
Bureau of Waste Management
1000 SW Jackson Street, Suite 400
Topeka, KS 66612-1367
Attention: Heather Merritt

RE: Ambient Air Monitoring Activities – 10/19/2026
City of Galena Construction and Demolition Landfill
KDHE Permit No. 738
Galena, Cherokee County, Kansas

Dear Ms. Merritt

Air monitoring was conducted on October 19, 2026, according to the Ambient Air Monitoring Protocol dated October 6, 2025, and approved by KDHE on October 29, 2025. The protocol, following Kansas Administrative Regulations (K.A.R.) 28-29-333(b)(1), included the use of a Jerome J605 to monitor hydrogen sulfide (H_2S) in parts per billion (ppb) and a Landtec GEM5000 to monitor methane (CH_4) concentrations as a percent of the lower explosive limit (LEL). These two instruments were calibrated prior to use, and a prevailing south-southeast wind determined the monitoring locations. A Kestrel 4000 was used on site as a handheld weather meter to determine wind speed, temperature, humidity, dew point, and barometric pressure. A handheld Garmin GPS device was utilized to document the location of each sampling event.

One location was monitored on the upwind (southeast) side of the landfill boundary as a background location, and a total of three additional locations were monitored downwind along the north and northwest sides of the property. The H_2S readings were taken every minute for 15 minutes, and the Time Weighted Average (TWA) was documented as the average of the 15 readings from each location. All sampling locations except the west-most downwind location (Sample ID 26101904) registered no detectable H_2S concentrations (≥ 0.003 ppm). Sample ID 26101904, located directly northwest of the landfill, exhibited an intermittent sulfur odor and individual (1-minute reading) concentrations ranging from 0.0 to 0.00583 throughout the 15-minute monitoring, leading to a TWA of 0.003464 ppm.

No sampling locations registered detectable methane concentrations above 0.0%. A site map is included as an attachment to this letter, and the tables attached below exhibit the air monitoring data (Table 1) and the location and weather conditions (Table 2) of each sampling location. Calibration certificates/reports for both the Jerome J605 and GEM5000 instruments are also included as attachments to this letter.


TriCore appreciates your time and consideration on this matter. If you have questions, comments, or need additional information, please do not hesitate to contact the undersigned.

Sincerely,

TriCore Group, LLC



Shane McKinzie



Joe Paul Edwards, P.E.

Attachments: Table 1: Ambient Air Monitoring Data
Table 2: Ambient Air Monitoring Location, Weather, and Observations
Figure 1: Air Monitoring Locations
Instrument Calibration Documents

Cc: Ashley Groves – City of Galena
Michelle Murphy – Jordan Disposal
Mads Gisselbaek – Jordan Disposal

C&D Landfill (No. 738) Ambient Air Monitoring Data

Table 1: Ambient Air Monitoring Data

Sample ID	Date	Time	Individual H ₂ S Readings															H ₂ S TWA	CH ₄
			01	02	03	04	05	06	07	08	09	10	11	12	13	14	15		
26101901	10/19/26	0750-0804	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	-	0.0
26101902	10/19/26	0830-0844	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	-	0.0
26101903	10/19/26	0849-0903	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	-	0.0
26101904	10/19/26	0908-0922	0.00462	0.00412	0.00510	0	0.00438	0.00323	0	0	0.00445	0.00539	0	0.00532	0.00475	0.00583	0.00477	0.003464	0.0
26101905	10/19/26	0953	0															n/a	0.0

*The H₂S (hydrogen sulfide) results are reported in parts per million (ppm).

**The CH₄ (methane) results are reported as a percentage of the lower explosive limit (LEL).

Table 2: Ambient Air Monitoring Location, Weather, and Observations

Sample ID	Date	Time	Latitude	Longitude	Wind Direction	Wind Speed (mph)	Temp. (F)	Humidity (%)	Dew Point	Barometric Pressure	Odor Observations
26101901	10/19/26	0802-0804	37.07863	-94.63060	SSE	2.2	53.5	52.6	36.6	29.33	Partly cloudy, no noticeable odor
26101902	10/19/26	0831-0833	37.08212	-94.63128	SSE	0.7	53.9	59.5	40.2	29.39	Partly cloudy, no noticeable odor
26101903	10/19/26	0849-0851	37.08223	-94.63379	SSE	4.0	57.8	50.8	39.7	29.38	Partly cloudy, intermittent light sulfur odor
26101904	10/19/26	0908-0910	37.08220	-94.63502	SSE	3.0	57.3	50.4	39.0	29.39	Mostly cloudy, intermittent sulfur odor
26101905	10/19/26	0931-0933	Scalehouse		n/a	n/a	n/a	n/a	n/a	n/a	No noticeable odor

*Each weather reading is reported as: Wind Speed = miles per hour, Temperature & Dew Point = degrees Fahrenheit, Humidity = percentage, and Barometric Pressure = inches of mercury


TriCore appreciates your time and consideration on this matter. If you have questions, comments, or need additional information, please do not hesitate to contact the undersigned.

Sincerely,

TriCore Group, LLC



Shane McKinzie



Joe Paul Edwards, P.E.

Attachments: Table 1: Ambient Air Monitoring Data
Table 2: Ambient Air Monitoring Location, Weather, and Observations
Figure 1: Air Monitoring Locations
Instrument Calibration Documents

Cc: Ashley Groves – City of Galena
Michelle Murphy – Jordan Disposal
Mads Gisselbaek – Jordan Disposal

C&D Landfill (No. 738) Ambient Air Monitoring Data

Table 1: Ambient Air Monitoring Data

Sample ID	Date	Time	Individual H ₂ S Readings															H ₂ S TWA	CH ₄
			01	02	03	04	05	06	07	08	09	10	11	12	13	14	15		
26101901	10/19/26	0750-0804	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	-	0.0
26101902	10/19/26	0830-0844	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	-	0.0
26101903	10/19/26	0849-0903	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	-	0.0
26101904	10/19/26	0908-0922	0.00462	0.00412	0.00510	0	0.00438	0.00323	0	0	0.00445	0.00539	0	0.00532	0.00475	0.00583	0.00477	0.003464	0.0
26101905	10/19/26	0953	0															n/a	0.0

*The H₂S (hydrogen sulfide) results are reported in parts per million (ppm).

**The CH₄ (methane) results are reported as a percentage of the lower explosive limit (LEL).

Table 2: Ambient Air Monitoring Location, Weather, and Observations

Sample ID	Date	Time	Latitude	Longitude	Wind Direction	Wind Speed (mph)	Temp. (F)	Humidity (%)	Dew Point	Barometric Pressure	Odor Observations
26101901	10/19/26	0802-0804	37.07863	-94.63060	SSE	2.2	53.5	52.6	36.6	29.33	Partly cloudy, no noticeable odor
26101902	10/19/26	0831-0833	37.08212	-94.63128	SSE	0.7	53.9	59.5	40.2	29.39	Partly cloudy, no noticeable odor
26101903	10/19/26	0849-0851	37.08223	-94.63379	SSE	4.0	57.8	50.8	39.7	29.38	Partly cloudy, intermittent light sulfur odor
26101904	10/19/26	0908-0910	37.08220	-94.63502	SSE	3.0	57.3	50.4	39.0	29.39	Mostly cloudy, intermittent sulfur odor
26101905	10/19/26	0931-0933	Scalehouse		n/a	n/a	n/a	n/a	n/a	n/a	No noticeable odor

*Each weather reading is reported as: Wind Speed = miles per hour, Temperature & Dew Point = degrees Fahrenheit, Humidity = percentage, and Barometric Pressure = inches of mercury

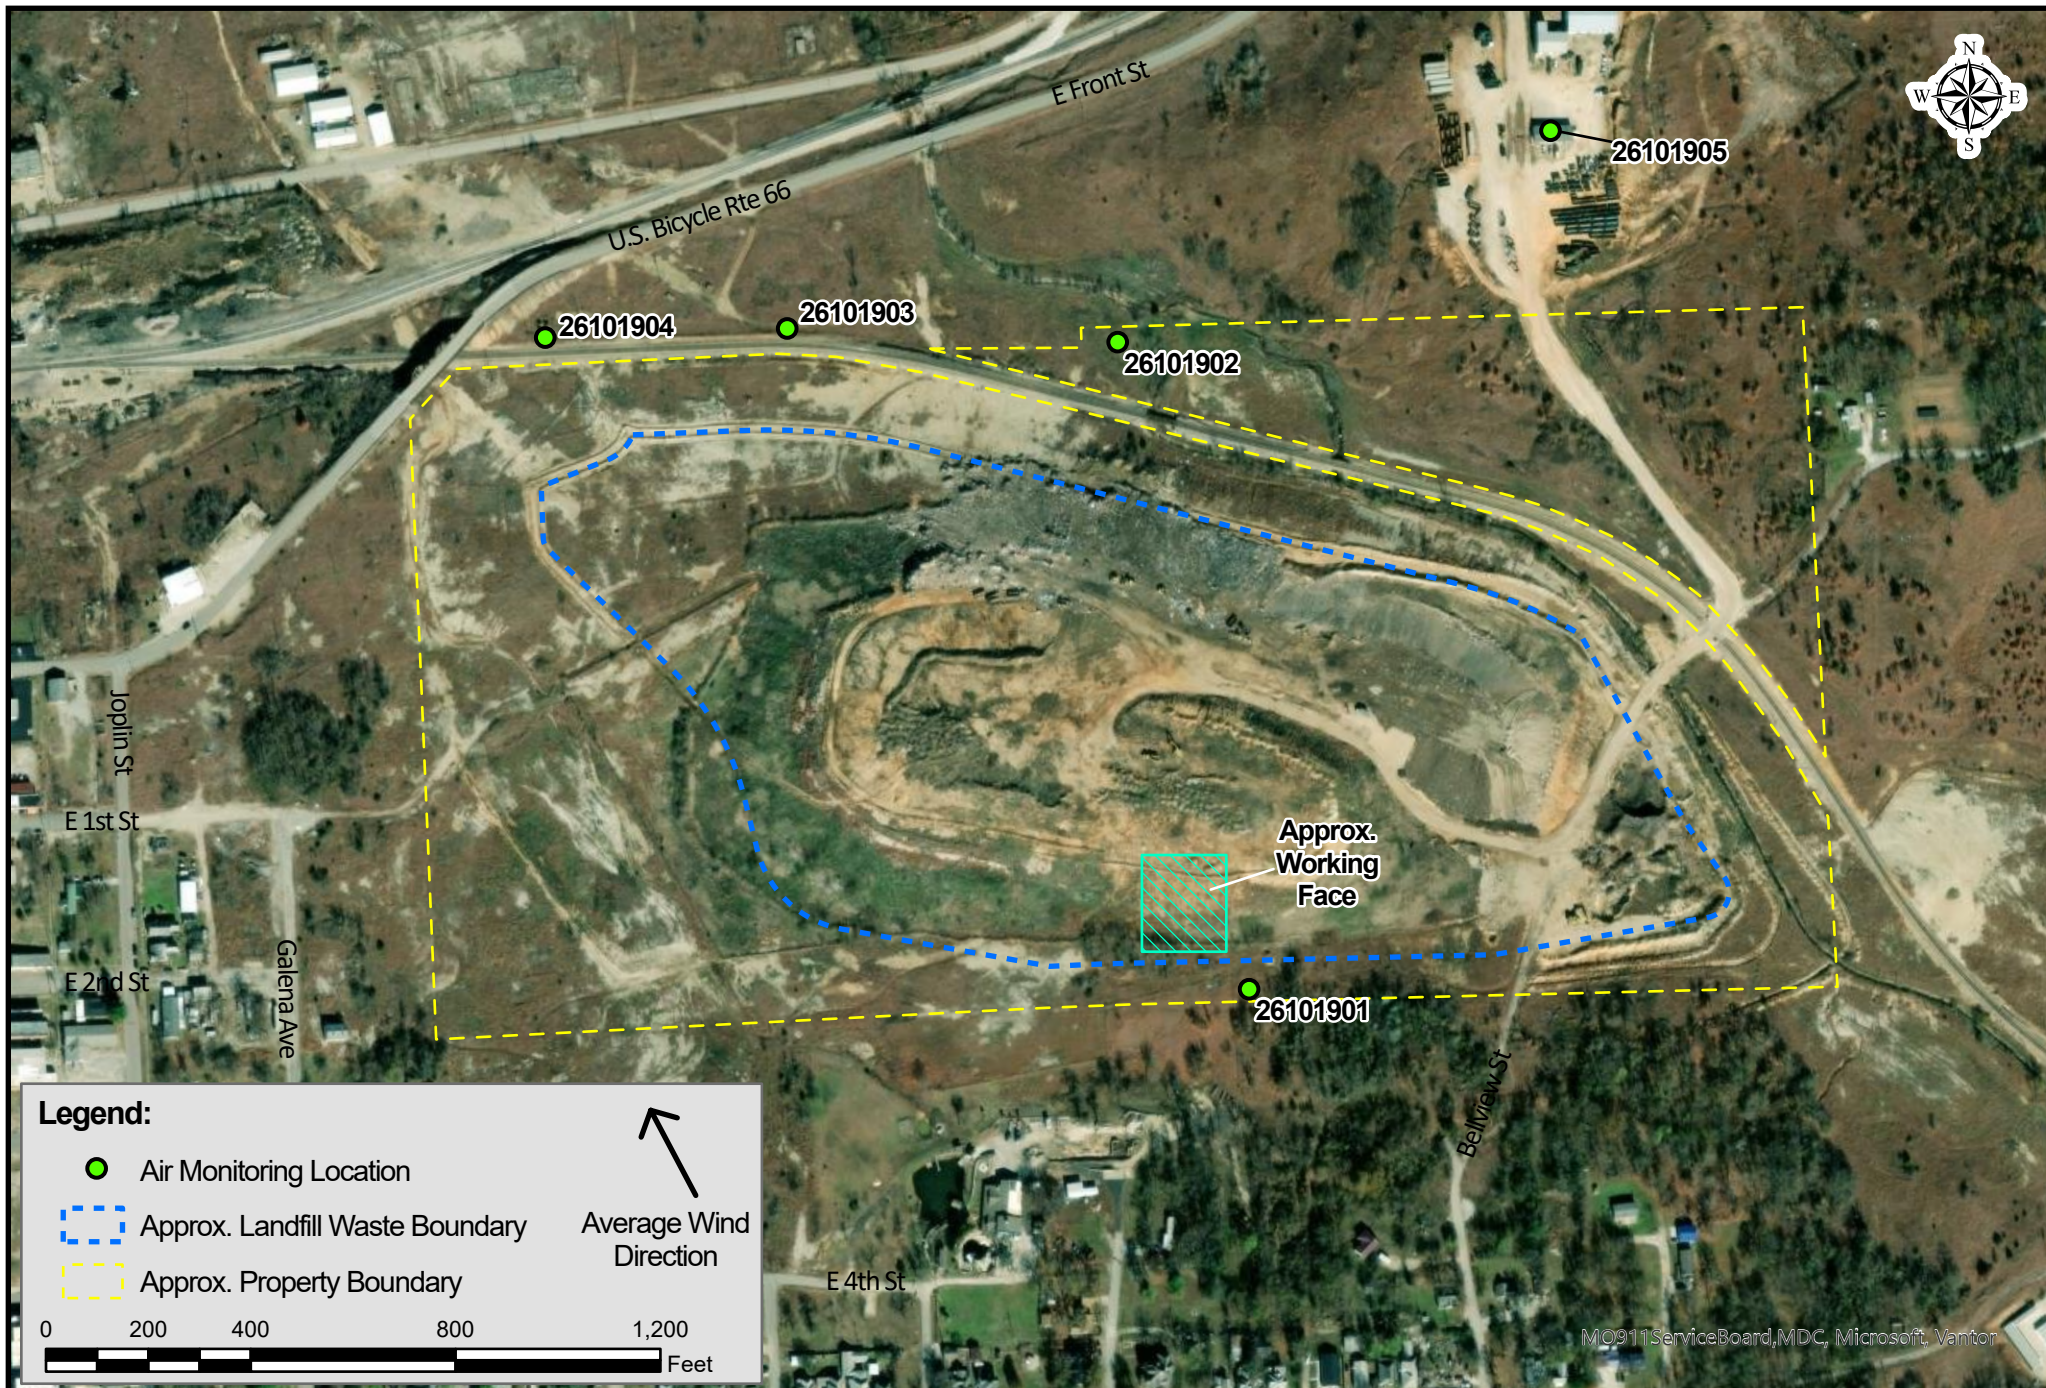


FIGURE 1
 AMBIENT AIR MONITORING
 JORDAN DISPOSAL LANDFILL
 AIR MONITORING LOCATIONS 10/19/26



TriCore Group, LLC
 PO Box 720992
 Oklahoma City, OK 73172
 405-256-2277
 www.tricoregrp.com

Address:
 1040 East Front Street
 Galena, KS 66739

County: Cherokee
 Lat: 37.083115
 Long: -94.62861

Drafted by SCM
 Drafted Date: 10/21/26
 Project #26C1KS-010



11 Commerce Blvd. | Middleboro, MA 02346
P: 508.946.6200 | F: 508.946.6262

CERTIFICATE NUMBER

392506

CUSTOMER NAME

CITY OF GALENA

ADDRESS211 W 7TH
GALENA KS 66739
USA**CERTIFICATE OF INSTRUMENT CALIBRATION**

<u>MODEL</u>	<u>SERIAL NUMBER</u>	<u>CALIBRATION DATE</u>	<u>CALIBRATION DUE DATE</u>
J605-0001	60500759	4/28/2026	4/27/2027

To the NATIONAL INSTITUTE OF STANDARDS AND TECHNOLOGY within the limitations of the Institute's calibration services, or have been derived from accepted values of natural physical constants, or have been derived by the ratio type of self-calibration techniques. Disclaimer: Any unauthorized adjustments, removal or breaking of QC seals, or other customer modifications on your Jerome Analyzer WILL VOID this factory calibration. Because any of the above acts could affect the calibration and readings of the instrument, their certification will no longer be valid and, further, AMETEK Brookfield WILL NOT be responsible for any liabilities created as a result of using the instrument after such adjustments, seal removal, or modifications. This document shall not be reproduced, except in full, without the written approval of AMETEK Brookfield.

REFERENCE EQUIPMENT USED TO CALIBRATE THE EQUIPMENT

<u>TYPE/MODEL</u>	<u>SERIAL/LOT NUMBER</u>	<u>CALIBRATION DATE</u>	<u>CALIBRATION DUE DATE</u>
Cal Set	CC240536	2/21/2024	2/21/2027

<u>TYPE/MODEL</u>	<u>SERIAL/LOT NUMBER</u>	<u>CALIBRATION DATE</u>	<u>CALIBRATION DUE DATE</u>
Alicat	60245	7/22/2025	7/23/2026

<u>TYPE/MODEL</u>	<u>SERIAL/LOT NUMBER</u>	<u>CALIBRATION DATE</u>	<u>CALIBRATION DUE DATE</u>
Alicat	437338	7/22/2025	7/23/2026

<u>TYPE/MODEL</u>	<u>SERIAL/LOT NUMBER</u>	<u>CALIBRATION DATE</u>	<u>CALIBRATION DUE DATE</u>
Fluke	84030258	9/12/2025	9/12/2026


NIST TRACE # SRM 2730; 65-D-035; CAL013399**PROCEDURE #:** 730-0099

All reference equipment used to calibrate the instrument listed upon this certificate have calibrations that are traceable to the National Institute of Standards and Technology (NIST).

APPROVAL SIGNATURE

TODD PLACE, QUALITY MANAGER

CALIBRATION PERFORMED BY MA

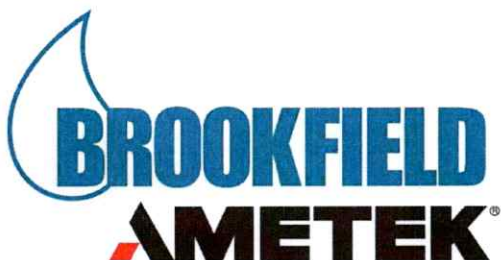

April 28, 2026
3375 N. Delaware Street, Chandler, AZ 85225
800.528.7411 Fax 602.281.1745
BrookfieldEngineering.com

J605 Incoming / Outgoing Data Sheet

MODEL

J605

SRO NUMBER

S211932

SERIAL NUMBER

60500759

INCOMING

Calibration Gas

	Allowable Range $\pm 6\%$	
	0.47 to 0.53 ppm H ₂ S	$\leq 3\%$
Concentration	Mean @ Saturation	Relative Standard Deviation
0.5000 ppm H ₂ S	0.0000 ppm H ₂ S	0.00%

Calibration Status as Received:

Functionally Unable to Check Calibration.

OUTGOING

Calibration Gas

	Allowable Range	
	0.47 to 0.53 ppm H ₂ S $\pm 6\%$	$\leq 5\%$
Concentration	Mean @ Saturation	Relative Standard Deviation
0.500 ppm H ₂ S	0.502 ppm H ₂ S	1.10%

Calibration Status as Left:

In Calibration.

Estimated Uncertainty of Calibration System: 3.5%



INSTRUMENT CALIBRATION REPORT

Pine Environmental Services LLC

11669 Lilburn Park Rd.
St. Louis, MO 63146
Office: 314.344.1079

Pine Environmental Services, Inc.

Instrument ID 44983
Description GEM5000
Calibrated 10/16/2026 2:51:51PM

Manufacturer CES Landtec
Model Number GEM5000
Serial Number/ Lot G506115
Number
Location St. Louis
Department

State Certified
Status Pass
Temp °C 22.2
Humidity % 43

Calibration Specifications							
Group # 1				Range Acc % 0.0000			
Group Name CH4				Reading Acc % 3.0000			
Stated Accy Pct of Reading				Plus/Minus 0.0			
<u>Nom In Val / In Val</u>	<u>In Type</u>	<u>Out Val</u>	<u>Out Type</u>	<u>Fnd As</u>	<u>Lft As</u>	<u>Dev%</u>	<u>Pass/Fail</u>
50.0 / 50.0	%Volume	50.0	%Volume	50.4	50.0	0.00%	Pass
Group # 2				Range Acc % 0.0000			
Group Name CO2				Reading Acc % 3.0000			
Stated Accy Pct of Reading				Plus/Minus 0.0			
<u>Nom In Val / In Val</u>	<u>In Type</u>	<u>Out Val</u>	<u>Out Type</u>	<u>Fnd As</u>	<u>Lft As</u>	<u>Dev%</u>	<u>Pass/Fail</u>
35.0 / 35.0	%Volume	35.0	%Volume	35.1	35.0	0.00%	Pass
Group # 3				Range Acc % 0.0000			
Group Name O2				Reading Acc % 3.0000			
Stated Accy Pct of Reading				Plus/Minus 0.0			
<u>Nom In Val / In Val</u>	<u>In Type</u>	<u>Out Val</u>	<u>Out Type</u>	<u>Fnd As</u>	<u>Lft As</u>	<u>Dev%</u>	<u>Pass/Fail</u>
20.9 / 20.9	%	20.9	%	20.2	20.9	0.00%	Pass
Group # 4				Range Acc % 0.0000			
Group Name H2S				Reading Acc % 3.0000			
Stated Accy Pct of Reading				Plus/Minus 0			
<u>Nom In Val / In Val</u>	<u>In Type</u>	<u>Out Val</u>	<u>Out Type</u>	<u>Fnd As</u>	<u>Lft As</u>	<u>Dev%</u>	<u>Pass/Fail</u>
50 / 50	PPM	50	PPM	50	50	0.00%	Pass
Group # 5				Range Acc % 0.0000			
Group Name CO				Reading Acc % 3.0000			
Stated Accy Pct of Reading				Plus/Minus 0			
<u>Nom In Val / In Val</u>	<u>In Type</u>	<u>Out Val</u>	<u>Out Type</u>	<u>Fnd As</u>	<u>Lft As</u>	<u>Dev%</u>	<u>Pass/Fail</u>
1000 / 1000	PPM	1000	PPM	1,033	1,000	0.00%	Pass

INSTRUMENT CALIBRATION REPORT



Pine Environmental Services LLC

11669 Lilburn Park Rd.
St. Louis, MO 63146
Office: 314.344.1079

Pine Environmental Services, Inc.

Instrument ID 44983
Description GEM5000
Calibrated 10/16/2026 2:51:51PM

<u>Test Instruments Used During the Calibration</u>					<u>(As Of Cal Entry Date)</u>	
<u>Test Standard ID</u>	<u>Description</u>	<u>Manufacturer</u>	<u>Model Number</u>	<u>Serial Number / Lot Number</u>	<u>Last Cal Date/ Opened Date</u>	<u>Next Cal Date / Expiration Date</u>
STL 50 CH4/35 CO2 L#304-4028832 4	STL 50 CH4/35 CO2 L#304-402883248-1	Gasco	X03ME50CP5000 0	304-402883248 -1		10/24/2027
STL GEM+ BLEND L#304-4036145 94-1	STL GEM+ BLEND L#304-403614594-1	Gasco	X03NI99CA34002 8	304-403614594 -1		4/22/2028
STL ZERO AIR L#304-4027967 63-1	STL ZERO AIR L#304-402796763-1	Gasco	AIUZP15	304-402796763 -1		9/6/2027

Notes about this calibration

Calibration Result Calibration Successful
Who Calibrated Chris Harkins

All instruments are calibrated by Pine Environmental Services LLC according to the manufacturer's specifications, but it is the customer's responsibility to calibrate and maintain this unit in accordance with the manufacturer's specifications and/or the customer's own specific needs.

Notify Pine Environmental Services LLC of any defect within 24 hours of receipt of equipment
Please call 800-301-9663 for Technical Assistance

CERTIFICATION OF CALIBRATION

Date Of Calibration: 30-Jan-2026



No. 66916



Certificate Number: G506115_10/40692

Issued by: QED Environmental Systems Inc.

Customer: PINE ENVIRONMENTAL SERVICES LLC
PO BOX 943 HIGHTSTOWN NJ 08520 UNITED STATES

Description:

Model: GEM5000

Serial Number: G506115

Accredited Results:

Methane (CH4)		
Certified Gas (%)	Instrument Reading (%)	Uncertainty (%)
5.0	4.9	0.42
15.0	14.9	0.66
60.0	59.6	1.03

Carbon Dioxide (CO2)		
Certified Gas (%)	Instrument Reading (%)	Uncertainty (%)
5.0	4.8	0.43
15.0	14.7	0.71
40.0	40.1	1.19

Oxygen (O2)		
Certified Gas (%)	Instrument Reading (%)	Uncertainty (%)
21.1	21.2	0.25

Gas cylinders are traceable and details can be provided if requested.

CH4, CO2 readings recorded at: 32.1 °C/89.7 °F

Barometric Pressure: 0992 mbar/29.30 "Hg

O2 readings recorded at: 23.4 °C/74.1 °F

Method of Test : The analyzer is calibrated in a temperature controlled chamber using a series of reference gases, in compliance with procedure ISP17.

Instrument has passed calibration as the measurement result is within the specification limit. The specification limit takes into account the measurement uncertainty.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor of k=2, providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with NIST requirements.

The calibration results published in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Certification only applies to results shown. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

Calibration Instance: 118

IGC Instance: 118

Page 1 of 3 | LP015LNANIST-1.1

www.qedenv.com (800) 624-2026 info@qedenv.com

QED Environmental Systems Inc. 2355 Bishop Circle West, Dexter, MI 48130

CERTIFICATION OF CALIBRATION

Date Of Calibration: 30-Jan-2026



No. 66916



Certificate Number: G506115_10/40692

Issued by: QED Environmental Systems Inc.

Non Accredited results:

Pressure Transducers (inches of water column)					
Transducer	Certified (Low)	Reading (Low)	Certified (High)	Reading (High)	Accuracy
Static	0"	0"	40"	40.16"	2.0"
Differential	0"	0"	4"	3.98"	0.7"

Barometer (mbar)	
Reference	Instrument Reading
0992 mbar / 29.30 "Hg	0993 mbar / 29.31 "Hg

Additional Gas Cells		
Gas	Certified Gas (ppm)	Instrument Reading (ppm)
H ₂ S	261	261
CO/H ₂ COMP	500	497

As received gas check readings:

Methane (CH ₄)	
Certified Gas (%)	Instrument Reading (%)
5.0	5.1
15.0	15.1
60.0	58.5

Carbon Dioxide (CO ₂)	
Certified Gas (%)	Instrument Reading (%)
5.0	5.3
15.0	15.7
40.0	41.4

Oxygen (O ₂)	
Certified Gas (%)	Instrument Reading (%)
21.1	20.9

As received Gas readings recorded at: 32.1 °C/89.7 °F

As received Barometric Pressure recorded at: 23.4 °C/74.1 °F

As received gas check readings are only recorded if the instrument is received in a working condition.

Where the instrument is received damaged no reading can be taken.

The calibration results published in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Certification only applies to results shown. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

Calibration Instance: 118

IGC Instance: 118

Page 2 of 3 | LP015LNANIST-1.1

www.qedenv.com (800) 624-2026 info@qedenv.com

QED Environmental Systems Inc. 2355 Bishop Circle West, Dexter, MI 48130

CERTIFICATION OF CALIBRATION

Date Of Calibration: 30-Jan-2026



No. 66916




Certificate Number: G506115_10/40692

Issued by: QED Environmental Systems Inc.

Date of Issue : 04 Feb 2026

Approved By Signatory

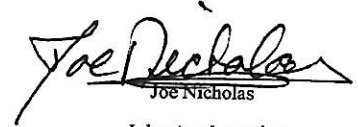
Joe Nicholas

Laboratory Inspection

The calibration results published in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Certification only applies to results shown. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

Calibration Instance: 118

IGC Instance: 118

Page 3 of 3 | LP015LNANIST-1.1

www.qedenv.com (800) 624-2026 info@qedenv.com

QED Environmental Systems Inc. 2355 Bishop Circle West, Dexter, MI 48130